

BAHAMAS NATIONAL STANDARD

**Medical devices – Quality management systems – Requirements
for regulatory purposes**

BNS ISO 13485:2016

Bahamas Bureau of Standards & Quality (BBSQ)
Source River Centre, 1000 Bacardi Road

P.O. Box N- 4843, Nassau, New Providence, Bahamas
Tel: (242) 362-1748 thru 56

Fax: (242) 362-9172

Email: standards@bbsq.bs

Website: www.bbsq.bs



FOR REVIEW ONLY

Website: www.bbsq.bs

© BBSQ – All rights reserved. No part of this publication is to be reproduced without the prior written consent of BBSQ.

ISBN 978-976-8268-20-4

NOTICE

Standards are subjected to periodic review.

The next amendment will be sent without charge if you return the self-addressed label. If we do not receive this label we have no record that you wish to be kept up-to-date. Please note amendments are not exclusive of a revision of the document.

Our address:

Bahamas Bureau of Standards & Quality (BBSQ)

Source River Centre

1000 Bacardi Road

P.O. Box N- 4843

Nassau, New Providence

Bahamas


----- (✂cut along the perforated line✂) -----

BNS ISO 13485:2016

NAME:

COMPANY/DESIGNATION:

ADDRESS:

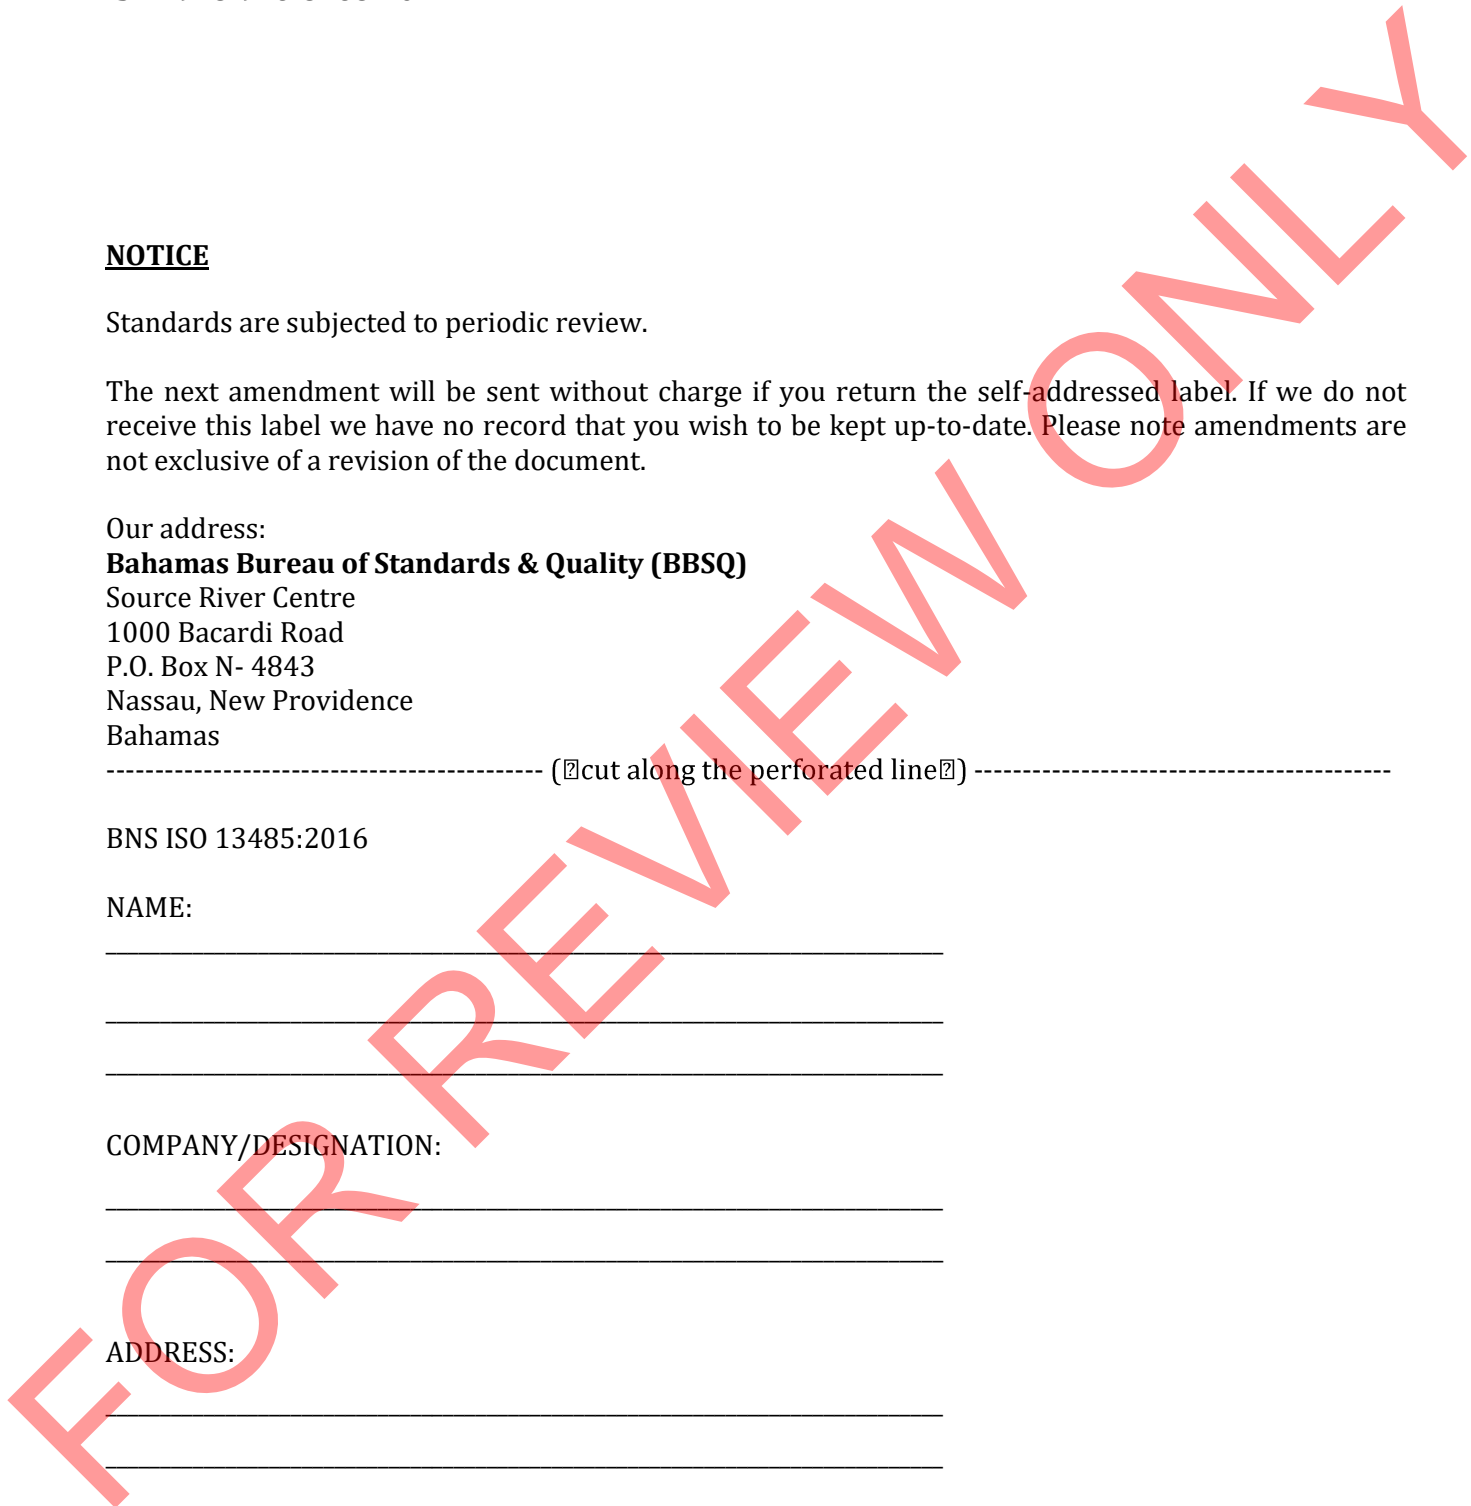

AMENDMENTS ISSUED SINCE PUBLICATION

AMENDMENT NO.	DATE OF ISSUE	TYPE OF AMENDMENT	NO. OF TEXT AFFECTED	TEXT OF AMENDMENT

FOR REVIEW ONLY

FOR REVIEW ONLY

ATTACHMENT PAGE FOR BNS AMENDMENT SHEETS

BBSQ Foreword

This national standard is identical with the English version of International Standard ISO 13485:2016, *Medical devices – Quality management systems – Requirements for regulatory purposes*. The national committee responsible for reviewing this standard is Technical Committee 8 *Laboratories*. This standard contains requirements that are relevant for The Bahamas.

BBSQ Committee Representation

This ISO International Standard was adopted as a National Standard under the supervision of the National Technical Committee for Laboratories (NTC 8) hosted by the Bahamas Bureau of Standards and Quality which at the time comprised the following members:

Member

Dr. Ismae Whyms – Chairperson
 Ms. Rachel Williams – Vice Chairperson
 Mr. Raymond Baillou – Technical Secretary

 Mrs. Bonaventia Culmer – Technical Secretary
 Ms. Ruth Munnings – Recording Secretary
 Mrs. Carole Neymour – Recording Secretary
 Mrs. Sybil Craigg- Bullard
 Mrs. Harriet Lundy
 Mr. Oslen Smith
 Ms. Bernice McClain
 Ms. Shenika Brown
 Ms. Shawania Davis
 Ms. Darnell Inniss
 Mrs. Veronica Ferguson
 Dr. Camille Stephen
 Mrs. Charlene Smith
 Mrs. Joan Armbrister
 Ms. Nicole Paul
 Ms. Claudia Ginton
 Mrs. Majorie Palmer – Newball
 Mr. Brian Beneby
 Dr. Indira Martin
 Ms. Shannon Barnett
 Dr. Yasmin Robinson

 Mrs. Margaret Daxon

Representing

PHA/ PMH LABS - Management & Quality
 Min. of Agriculture & Marine Resources
 Quality Assured Laboratory Services (QALS) Partners
 Bonaventure Medical Laboratory
 Min. of Environment & Housing
 Bahamas Medical Laboratory Services
 N/A
 Doctors Hospital Laboratory Services
 Water & Sewerage Corporation
 Chest Center Laboratory
 ADKA Laboratories
 ADKA Laboratories
 Caribbean Health
 RBPF - Lab (Scientific Support Services)
 PMH-LAB
 Aquapure Ltd.
 GBHS
 GBHS
 GBHS
 PMH-LAB
 Water & Sewerage Corporation
 Min. of Health - Reference Labs
 Min. of Health - Reference Labs
 The Hospitals & Health Care Facilities Licensing Board
 The Hospitals & Health Care Facilities Licensing Board

Contents	Page
Foreword	viii
Introduction	ix
2 Scope	1
3 Normative references	1
4 Terms and definitions	2
5 Quality management system	7
5.1 General requirements	7
5.2 Documentation requirements	8
6 Management responsibility	10
6.1 Management commitment	10
6.2 Customer focus.....	11
6.3 Quality policy	11
6.4 Planning.....	11
6.5 Responsibility, authority and communication	11
6.6 Management review	12
7 Resource management	13
7.1 Provision of resources	13
7.2 Human resources	13
7.3 Infrastructure	13
7.4 Work environment and contamination control	14
8 Product realization	14
8.1 Planning of product realization	14
8.2 Customer-related processes.....	15
8.3 Design and development	16
8.4 Purchasing.....	19
8.5 Production and service provision.....	20
8.6 Control of monitoring and measuring equipment.....	24
9 Measurement, analysis and improvement	25
9.1 General.....	25
9.2 Monitoring and measurement.....	25
9.3 Control of nonconforming product	27
9.4 Analysis of data	28
9.5 Improvement	28
Annex A (informative) Comparison of content between ISO 13485:2003 and ISO 13485:2016 ..	30
Annex B (informative) Correspondence between ISO 13485:2016 and ISO 9001:2015	34
Bibliography	41

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT) see the following URL: www.iso.org/iso/foreword.html.

The committee responsible for this document is Technical Committee ISO/TC 210, *Quality management and corresponding general aspects for medical devices*.

This third edition of ISO 13485 cancels and replaces the second edition (ISO 13485:2003) and ISO/TR 14969:2004, which have been technically revised. It also incorporates the Technical Corrigendum ISO 13485:2003/Cor.1:2009. A summary of the changes incorporated into this edition compared with the previous edition is given in Annex A.

Introduction

0.1 General

This International Standard specifies requirements for a quality management system that can be used by an organization involved in one or more stages of the life-cycle of a medical device, including design and development, production, storage and distribution, installation, servicing and final decommissioning and disposal of medical devices, and design and development, or provision of associated activities (e.g. technical support). The requirements in this International Standard can also be used by suppliers or other external parties providing product (e.g. raw materials, components, subassemblies, medical devices, sterilization services, calibration services, distribution services, maintenance services) to such organizations. The supplier or external party can voluntarily choose to conform to the requirements of this International Standard or can be required by contract to conform.

Several jurisdictions have regulatory requirements for the application of quality management systems by organizations with a variety of roles in the supply chain for medical devices. Consequently, this International Standard expects that the organization:

- identifies its role(s) under applicable regulatory requirements;
- identifies the regulatory requirements that apply to its activities under these roles;
- incorporates these applicable regulatory requirements within its quality management system.

The definitions in applicable regulatory requirements differ from nation to nation and region to region. The organization needs to understand how the definitions in this International Standard will be interpreted in light of regulatory definitions in the jurisdictions in which the medical devices are made available.

This International Standard can also be used by internal and external parties, including certification bodies, to assess the organization's ability to meet customer and regulatory requirements applicable to the quality management system and the organization's own requirements. It is emphasized that the quality management system requirements specified in this International Standard are complementary to the technical requirements for product that are necessary to meet customer and applicable regulatory requirements for safety and performance.

The adoption of a quality management system is a strategic decision of an organization. The design and implementation of an organization's quality management system is influenced by the:

- a) organizational environment, changes in that environment, and the influence that the organizational environment has on the conformity of the medical devices;
- b) organization's varying needs;
- c) organization's particular objectives;
- d) product the organization provides;
- e) processes the organization employs;
- f) organization's size and organizational structure;
- g) regulatory requirements applicable to the organization's activities.

It is not the intent of this International Standard to imply the need for uniformity in the structure of different quality management systems, uniformity of documentation or alignment of documentation to the clause structure of this International Standard.

There is a wide variety of medical devices and some of the particular requirements of this International Standard only apply to named groups of medical devices. These groups are defined in Clause 3.

FOR REVIEW ONLY

0.2 Clarification of concepts

In this International Standard, the following terms or phrases are used in the context described below.

- When a requirement is qualified by the phrase “as appropriate”, it is deemed to be appropriate unless the organization can justify otherwise. A requirement is considered appropriate if it is necessary for:
 - product to meet requirements;
 - compliance with applicable regulatory requirements;
 - the organization to carry out corrective action;
 - the organization to manage risks.
- When the term “risk” is used, the application of the term within the scope of this International Standard pertains to safety or performance requirements of the medical device or meeting applicable regulatory requirements.
- When a requirement is required to be “documented”, it is also required to be established, implemented and maintained.
- When the term “product” is used, it can also mean “service”. Product applies to output that is intended for, or required by, a customer, or any intended output resulting from a product realization process.
- When the term “regulatory requirements” is used, it encompasses requirements contained in any law applicable to the user of this International Standard (e.g. statutes, regulations, ordinances or directives). The application of the term “regulatory requirements” is limited to requirements for the quality management system and the safety or performance of the medical device.

In this International Standard, the following verbal forms are used:

- “shall” indicates a requirement;
- “should” indicates a recommendation;
- “may” indicates a permission;
- “can” indicates a possibility or a capability.

Information marked as “NOTE” is for guidance in understanding or clarifying the associated requirement.

0.3 Process approach

This International Standard is based on a process approach to quality management. Any activity that receives input and converts it to output can be considered as a process. Often the output from one process directly forms the input to the next process.

For an organization to function effectively, it needs to identify and manage numerous linked processes. The application of a system of processes within an organization, together with the identification and interactions of these processes, and their management to produce the desired outcome, can be referred to as the “process approach.”

When used within a quality management system, such an approach emphasizes the importance of:

- a) understanding and meeting requirements;

- b) considering processes in terms of added value;
- c) obtaining results of process performance and effectiveness;
- d) improving processes based on objective measurement.

FOR REVIEW ONLY

0.4 Relationship with ISO 9001

While this is a stand-alone standard, it is based on ISO 9001:2008, which has been superseded by ISO 9001:2015. For the convenience of users, Annex B shows the correspondence between this International Standard and ISO 9001:2015.

This International Standard is intended to facilitate global alignment of appropriate regulatory requirements for quality management systems applicable to organizations involved in one or more stages of the life-cycle of a medical device. This International Standard includes some particular requirements for organizations involved in the life-cycle of medical devices and excludes some of the requirements of ISO 9001 that are not appropriate as regulatory requirements. Because of these exclusions, organizations whose quality management systems conform to this International Standard cannot claim conformity to ISO 9001 unless their quality management system meets all the requirements of ISO 9001.

0.5 Compatibility with other management systems

This International Standard does not include requirements specific to other management systems, such as those particular to environmental management, occupational health and safety management, or financial management. However, this International Standard enables an organization to align or integrate its own quality management system with related management system requirements. It is possible for an organization to adapt its existing management system(s) in order to establish a quality management system that complies with the requirements of this International Standard.

FOR REVIEW ONLY

Medical devices – Quality management systems – Requirements for regulatory purposes

1 Scope

This International Standard specifies requirements for a quality management system where an organization needs to demonstrate its ability to provide medical devices and related services that consistently meet customer and applicable regulatory requirements. Such organizations can be involved in one or more stages of the life-cycle, including design and development, production, storage and distribution, installation, or servicing of a medical device and design and development or provision of associated activities (e.g. technical support). This International Standard can also be used by suppliers or external parties that provide product, including quality management system-related services to such organizations.

Requirements of this International Standard are applicable to organizations regardless of their size and regardless of their type except where explicitly stated. Wherever requirements are specified as applying to medical devices, the requirements apply equally to associated services as supplied by the organization.

The processes required by this International Standard that are applicable to the organization, but are not performed by the organization, are the responsibility of the organization and are accounted for in the organization's quality management system by monitoring, maintaining, and controlling the processes.

If applicable regulatory requirements permit exclusions of design and development controls, this can be used as a justification for their exclusion from the quality management system. These regulatory requirements can provide alternative approaches that are to be addressed in the quality management system. It is the responsibility of the organization to ensure that claims of conformity to this International Standard reflect any exclusion of design and development controls.

If any requirement in Clauses 6, 7 or 8 of this International Standard is not applicable due to the activities undertaken by the organization or the nature of the medical device for which the quality management system is applied, the organization does not need to include such a requirement in its quality management system. For any clause that is determined to be not applicable, the organization records the justification as described in 4.2.2.

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 9000:2015¹, *Quality management systems — Fundamentals and vocabulary*

¹ Supersedes ISO 9000:2005.